
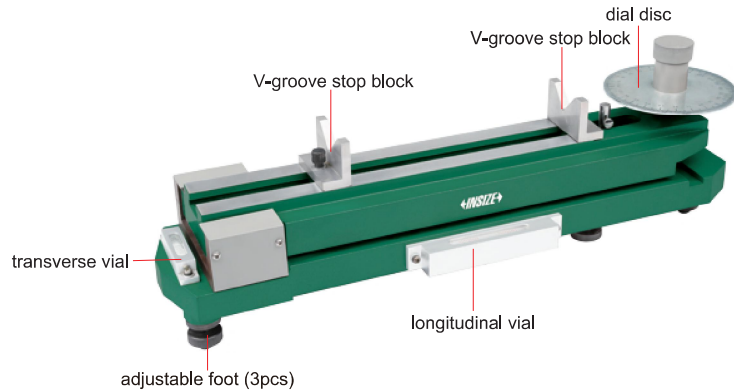


LEVEL CALIBRATOR

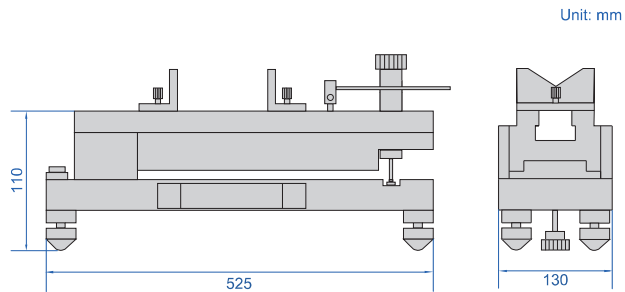

4960-1A

- With transverse vial and longitudinal vial, longitudinal vial graduation: 0.02mm/m

Code	Range	Graduation	Graduation accuracy	Hysteresis
4960-1A	0-1mm/m	0.005mm/m	0.0003mm/m	0.0025mm/m